


Calibration Checker

For Ground Tester Models 6422/6424

The Calibration Checker provides two test resistances (25 Ω and 125 Ω) to check the accuracy of your Model 6422 or 6424.

1. Insert the Calibration Checker into the instrument's terminals. Ensure each pin is inserted in its corresponding terminal (H-S-E).

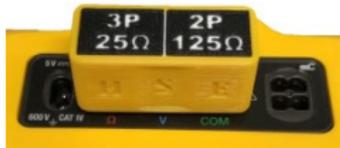

2. Observe the reading. This should be 125 $\Omega \pm 2.7\Omega$.



3. Press **TEST**. After a few moments the reading appears. This should be 25 $\Omega \pm 0.35\Omega$.



Technical and Sales Assistance

If you are experiencing any technical problems, or require any assistance with starting, configuring, or operating your instrument, please call, mail, fax or e-mail our technical support team:

Chauvin Arnoux[®], Inc. d.b.a. AEMC[®] Instruments

Phone: (800) 343-1391
(508) 698-2115

Fax: (508) 698-2118

E-mail: techsupport@aemc.com

www.aemc.com