
BATTERY REPLACEMENT PROCEDURE

POWER & ENERGY LOGGERS MODELS PEL 102 & PEL 103

(Battery for Cat. #'s 2137.51, 2137.52, 2137.61, 2137.62)

The Power & Energy Loggers PEL 102/103 include an 8.4V NiHM battery pack (**Cat. #2137.81**) for backup power. This battery, shown below, can be replaced by the user. With normal use, the battery should only need to be replaced approximately once every three or four years. This battery is available for purchase directly on our storefront at: <http://www.aemc.com/store>.



**IMPORTANT WARNING!**

The PEL battery replacement must be performed carefully and in strict accordance with the procedure described in this manual. Any variation could result in damage to the instrument and may void your warranty. *If you are unsure about performing this procedure, return the PEL to AEMC® for a factory battery replacement.*

Before You Begin

To replace the battery in the PEL, you will need the following:

- A clean work surface free of debris, water, and other possible contaminants. This surface should be well-lighted and provide sufficient room to perform the steps below.
- 8.4V NiHM battery pack.
- Torx T10 screwdriver (Torx type screwdrivers are also known as “star” screwdrivers)
- Tape (masking, electrical, etc.)
- (Optional) A small non-conducting implement such as a drink stirring stick or toothpick

Before starting this procedure, we recommend that you view the instructional video “PEL 102/103 Battery Replacement” on our [AEMC YouTube channel](#).

Note that the battery pack shown in the following illustrations may differ in color from your battery. However, the steps in the procedure are identical.

Battery Replacement Procedure

To replace the battery in the PEL 102/103, disconnect the instrument from all electrical sources and sensor probes. Then follow these steps:

1. Apply tape to the control buttons on the PEL front panel (see Figure 1). This tape will ensure that the buttons remain in place when you remove the PEL's front cover from the back cover.
2. Tape the PEL's endplates to the back cover (see Figure 2). This helps ensure that the endplates remain attached to the back cover when you remove the front cover.



Figure 1



Figure 2

3. Turn over the PEL, and locate the six fastening screws on the back of the instrument.



Figure 3

4. Using a Torx T10 screwdriver, remove these fastening screws.
5. Carefully separate the front cover of the PEL from the back cover. Typically, the two covers fit together very snugly, so it may be difficult at first to separate them.

One way to do this is to turn the instrument on its side as shown in Figure 4, and then carefully separate each corner in turn, starting with the bottom right corner. With your fingers on

the bottom endplate, pull the covers apart, ensuring that the endplate remains attached to the back cover.

CAUTION: Do not allow either the top or bottom endplate to become separated from the back cover. This may cause damage to the input and connection terminals, requiring that the PEL be sent to AEMC for repair.



Figure 4

6. With the front cover removed, locate the battery pack.



Figure 5

7. Gently remove and unplug the battery from the PEL. A small non-conductive implement such as a drink stirring stick (shown below) can be useful for doing this.

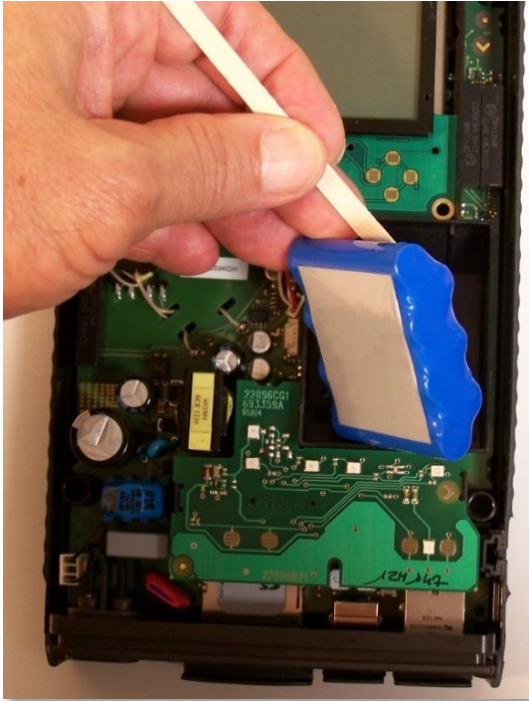


Figure 6

8. Inspect the plug of the replacement battery back, and note the position of the connector pins.



Figure 7

9. Position the plug with the connector pins facing away from the battery pack compartment. In the illustration below, the pins are facing towards the left. Then very carefully insert the plug by gently pushing it into the socket within the PEL. There is very little room for this procedure, so an implement such as a stirring stick or toothpick may be helpful in ensuring the plug is securely inserted. (The PEL instrument will likely turn on when you plug in the connector; this can be disregarded.)

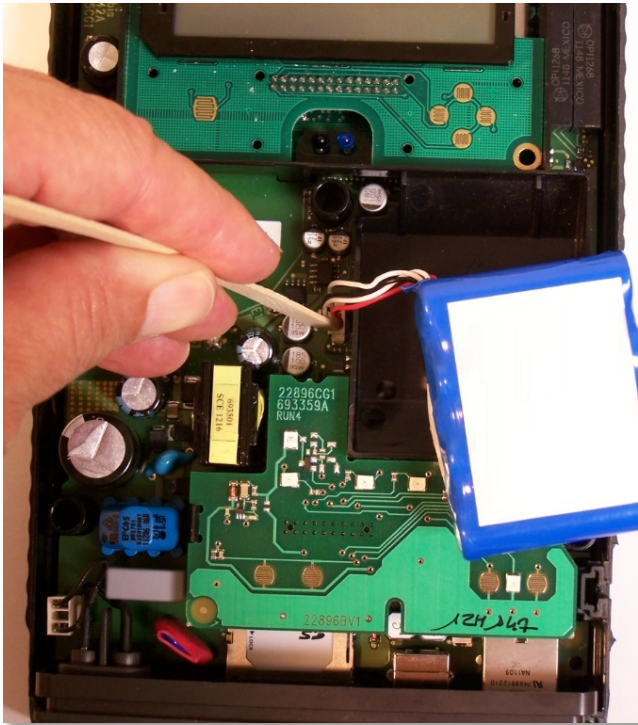


Figure 8

- Place the replacement battery into the compartment provided for it within the PEL. When doing this, ensure that the battery's connector wires are positioned as shown in the first illustration below. **Be sure the wires do not cross over the top of the post, as shown in the second illustration below. If the wires are placed over the post, they will likely be damaged when you replace the PEL top cover.**

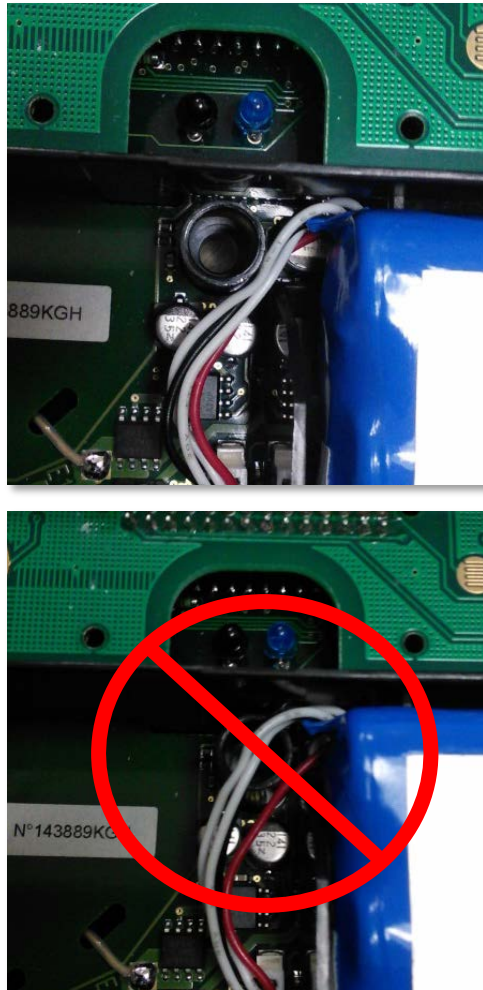


Figure 9

11. Replace the front cover, carefully ensuring that it is securely in place.
12. Turn the PEL over, and replace the six fastening screws removed in step 3 of this procedure.
13. Remove the tape applied to the front cover and endplates at the beginning of this procedure. The PEL is now ready for operation.



Chauvin Arnoux®. Inc. d.b.a. AEMC® Instruments
15 Faraday Drive • Dover, NH 03820 USA
Phone: (603) 749-6434 • (800) 945-2362
Fax: (603) 742-2346
www.aemc.com